


090417 XRD Quiz 2

- 1) Sketch an X-ray tube showing the a) source of electrons, b) source of X-rays, and c) explain how the two knobs on the front of the X-ray generator control the X-ray output in the tube.
- 2) a) Explain the difference between bremsstrahlung radiation, white radiation and the continuous spectrum. b) Are these radiations made in an X-ray tube? c) How or Why?
- 3) a) What is the dependence of X-ray absorption coefficient on wavelength? b) In order to calculate the thickness of lead needed to shield an X-ray generator using a copper target and running at 20 mA and 50 kV what wavelength would you use to determine the absorption coefficient.
- 4) a) If the intensity of diffracted X-rays is proportional to the thickness of the sample, for a pinhole measurement, and the diffracted X-rays must obey Beer's Law, show how you can determine the optimum thickness for a transmission sample. b) If the optimum thickness for a polymer sample is 2 mm what is the linear absorption coefficient?
- 5) For a copper anode show a plot of intensity versus wavelength (the emission spectrum) for an X-ray tube for excitation at 3kV 100 mA; 6kV 100 mA; and 30 kV 100 mA. Give the wavelength of the characteristic lines and of the short wavelength limit as well as the relative intensity of the characteristic lines for $K\alpha$ and $K\beta$ radiation.

ANSWERS: 061004 XRD Quiz 2

- 1) Filament at the top is the source of electrons. The target (anode) at the bottom is the source of X-rays. The voltage knob adjusts the potential drop from the filament to the anode. The current knob adjusts the tube current from the filament to the anode through a servo controller that adjusts the filament current.

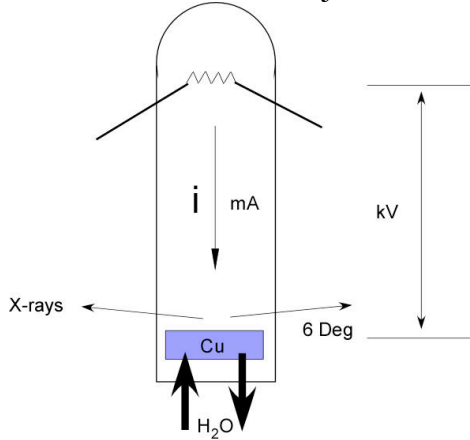

- 2) a) Bremsstrahlung, white and continuous radiation are the same thing. b) c) This refers to the spectrum produced by electrons as they impact the target (anode) atoms and convert their momentum to X-rays in the process. Yes they are made in the X-ray tube.
- 3) a) $\mu = k \rho \lambda^3 Z^3$ between absorption edges. At the absorption edge the coefficient drops in a step manner
 b) $\lambda_{SWL} = 12.4/50kV = 0.25 \text{ \AA}$. This is the highest energy radiation to shield.
- 4) a) $I_{\text{diffraction}} = C \times \exp(-\mu x)$. At the optimal thickness, x^* , $dI_{\text{diffraction}}/dx = 0$.
 $dI_{\text{diffraction}}/dx = C(\exp(-\mu x^*) - \mu x^* \exp(-\mu x^*)) = 0$
 or
 $1 - \mu x^* = 0$
 so
 $x^* = 1/\mu$.
 b) 0.5 mm^{-1}
- 5) $\lambda_{SWL,3kV} = 12.4/3kV = 4.1 \text{ \AA}$; $\lambda_{SWL,6kV} = 12.4/6kV = 2.1 \text{ \AA}$; $\lambda_{SWL,30kV} = 12.4/30kV = 0.41 \text{ \AA}$
 $\lambda_{K\alpha} = 1.54 \text{ \AA}$ and $\lambda_{K\beta} = 1.4 \text{ \AA}$ and these are about 100x and 20x the intensity of the white radiation.

